

Original citation:

McKelvey, Kim M. (Kim Martin), Nadappuram, Binoy Paulose, Actis, Paolo, Takahashi, Yasufumi, Korchev, Yuri E., Matsue, Tomokazu, Robinson, Colin and Unwin, Patrick R.. (2013) Fabrication, characterization, and functionalization of dual carbon electrodes as probes for scanning electrochemical microscopy (SECM). *Analytical Chemistry*, Volume 85 (Number 15). pp. 7519-7526.

Permanent WRAP url:

<http://wrap.warwick.ac.uk/57254>

Copyright and reuse:

The Warwick Research Archive Portal (WRAP) makes this work of researchers of the University of Warwick available open access under the following conditions. Copyright © and all moral rights to the version of the paper presented here belong to the individual author(s) and/or other copyright owners. To the extent reasonable and practicable the material made available in WRAP has been checked for eligibility before being made available.

Copies of full items can be used for personal research or study, educational, or not-for-profit purposes without prior permission or charge. Provided that the authors, title and full bibliographic details are credited, a hyperlink and/or URL is given for the original metadata page and the content is not changed in any way.

Publisher's statement:

This document is the Accepted Manuscript version of a Published Work that appeared in final form in *Analytical Chemistry* copyright © American Chemical Society after peer review and technical editing by the publisher. To access the final edited and published work <http://dx.doi.org/10.1021/ac401476z>

The version presented here may differ from the published version or, version of record, if you wish to cite this item you are advised to consult the publisher's version. Please see the 'permanent WRAP url' above for details on accessing the published version and note that access may require a subscription.

For more information, please contact the WRAP Team at: publications@warwick.ac.uk

warwick**publications**wrap

highlight your research

<http://wrap.warwick.ac.uk/>

Fabrication, Characterization and Functionalization of Dual Carbon Electrodes as Probes for Scanning Electrochemical Microscopy (SECM)

Kim McKelvey,^{a,b,c} Binoy Paulose Nadappuram,^b Paolo Actis,^d Yasufumi Takahashi,^e
Yuri E. Korchev,^d Tomokazu Matsue,^{e,f} Colin Robinson,^c Patrick R. Unwin^{b*}

^aMolecular Organisation and Assembly in Cells (MOAC) Doctoral Training Centre,

^bDepartment of Chemistry and ^cSchool of Life Sciences, University of Warwick, Coventry,
U.K. CV4 7AL.

^dDivision of Medicine, Imperial College London, London, U.K. W12 0NN

^eWorld Premier International Research Center-Advanced Institute for Materials Research,
Tohoku University, Katahira, Aoba 2-1-1, Sendai 980-8577, Japan

^fGraduate School of Environmental Studies, Tohoku University, 6-6-11 Aramaki Aoba,
Sendai 980-8579, Japan

*P.R.Unwin@warwick.ac.uk

Abstract

Dual carbon electrodes (DCEs) are quickly, easily and cheaply fabricated by depositing pyrolytic carbon into a quartz theta nanopipet. The size of DCEs can be controlled by adjusting the pulling parameters used to make the nanopipet. When operated in generation/collection (G/C) mode, the small separation between the electrodes leads to reasonable collection efficiencies of ca. 30 %. A 3 dimensional finite element method (FEM) simulation is developed to predict the current response of these electrodes as a means of estimating the probe geometry. Voltammetric measurements at individual electrodes combined with generation/collection measurements provide a reasonable guide to the electrode size. DCEs are employed in a scanning electrochemical microscopy (SECM) configuration and their use for both approach curves and imaging is considered. G/C approach curve measurements are shown to be particularly sensitive to the nature of the substrate, with insulating surfaces leading to enhanced collection efficiencies, whereas conducting surfaces lead to a decrease of collection efficiency. As a proof-of-concept, DCEs are further used to locally generate an artificial electron acceptor and to follow the flux of this species and its reduced form, during photosynthesis at isolated thylakoid membranes. In addition, 2 dimensional images of a single thylakoid membrane are reported and analyzed, to demonstrate the high sensitivity of G/C measurements to localized surface processes. It is finally shown that individual nanometer-size electrodes can be functionalized, through the selective deposition of platinum on one of the two electrodes in a DCE while leaving the other one unmodified. This provides an indication of the future versatility of this type of probe for nanoscale measurements and imaging.

Introduction

Ultramicroelectrodes (UMEs) offer high mass transport rates, low ohmic (IR) effects, low double layer charging,¹⁻³ and, as such, are optimal for many applications from kinetic measurements to electrochemical imaging. UMEs serve as imaging probes in scanning electrochemical microscopy (SECM), which has been used widely to study interfacial process at the microscale and nanoscale, especially electrocatalysis⁴⁻⁶ and in biological systems.⁷⁻¹² However, the overwhelming majority of these systems use single electrode probes and SECM can be productively extended to increasingly complex and challenging systems through the use of dual electrode probes. In principle, such probes would allow two redox-active species to be detected concurrently or would permit redox-active species to be generated at one electrode and collected at the other electrode.^{13,14}

Dual electrode systems are widely used to study the kinetics of redox reactions.^{15,16} Usually, but not exclusively,^{17,32} such devices operate in an amperometric/voltammetric mode, where each electrode is held at a potential to oxidize or reduce a target species of interest, and the current measured at each electrode relates to the flux of that active species arriving at the electrode. In generation/collection (G/C) mode, one electrode generates the species of interest (oxidizes or reduces the analyte (A) to produce an active species (S1)) that is then collected at the other electrode (via oxidation or reduction to produce the starting material or another species (S2)):



The flux of active species generated and collected depends on the geometry of the dual electrode system and the mass transport between the electrodes. The G/C mode is often characterized by the collection efficiency, N , which is defined as the ratio of the current

measured at the collector electrode to that measured at the generator electrode, usually under steady state conditions.

Dual electrode systems that are constructed in a probe-type configuration include ring-disk,^{18,19} dual-ring²⁰ and dual-disk^{21–24} geometries. Probe-based dual electrode systems have been constructed using single and dual barrel (theta) borosilicate and quartz pipets as a scaffold.^{21,25} However, collection efficiencies for the majority of these systems have been low because the inter-electrode distance has often been large with respect to the electrode size. A range of electrode sizes from 50 μm ²¹ to nanometers²³ have been reported, but the wider adoption of these systems has been limited due to difficulties in fabricating and characterizing the probes.

Herein, we present a quick and simple method for the fabrication of probe-based dual carbon electrodes (DCEs). This method allows the reproducible fabrication of a wide range of DCE sizes (from nanoscale to microscale). DCEs are prepared from a laser-pulled quartz theta pipet followed by pyrolytic carbon deposition. This is a development of a recent method reported for making scanning ion conductance–scanning electrochemical microscopy (SICM-SECM) probes.²⁵ Pyrolytic deposition of carbon to form electrodes is a popular method, employed to form several different SECM probes.^{20,26,27,28}

Nanoscale DCEs are rather challenging to characterize geometrically.^{29–31} As part of this study we therefore developed a finite element method (FEM) simulation that allowed the effective geometry of individual nanoscale probes to be estimated from single barrel voltammetry and G/C measurements. Furthermore, to demonstrate the suitability of these probes for SECM and to provide further insight into the probe geometry, approach curves, to insulating (inert) and conductive (active) surfaces, were recorded in probe G/C mode using intermittent contact-SECM (IC-SECM).^{32–35}

As a proof-of-concept, we used DCEs to study photosynthesis, at a film of isolated thylakoid membranes. In higher plants, thylakoid membranes contain the light dependent components of photosynthesis, at which light is absorbed and used to split water (at photosystem II).³⁶ Electrons, produced from the splitting of water, are transferred through the linear electron transport pathway before being used to produce the energy rich molecule, NADPH.³⁶ Interestingly, a number of artificial electron acceptors can intercept the electrons and be reduced by various components of this thylakoid membrane-bound electron transport pathway.^{36,37} We use a DCE to locally generate an artificial electron acceptor (oxidizing ferrocenylmethyl trimethylammonium, FcTMA^+ , to produce FcTMA^{2+}) and to monitor local flux of both species. The SECM platform also allowed us to construct 2D current images of a single thylakoid membrane, highlighting the subtle interactions of a locally generated electron acceptor with a dynamic biological membrane.

Finally, we show that individual electrodes within a single probe can be functionalized, through the selective deposition of platinum. This demonstrates that DCEs could be used as a platform for a range of chemical sensing applications in the future.

Experimental

Materials and reagents, together with details of the protocols used to prepare thylakoid membranes, are detailed in Supporting Information, S1-S3.

Electrode fabrication. DCEs were fabricated by adapting the method previously described by Takahashi et al.²⁵ Quartz theta pipets (O.D. 1.2 mm, I.D. 0.9 mm, Intracell) were pulled using a laser puller (P-2000, Sutter Instruments); see Supporting Information, section S4, for pulling parameters. Butane was passed through the pulled pipet, via tubing, under an argon atmosphere. The tip of the probe was heated with a butane torch for 35 s, to pyrolytically deposit carbon from the butane, as illustrated in Figure 1 A. Electrical contact to

each electrode was established by inserting a copper wire through the top end of the pipet barrel to make contact with the carbon layers. A field-emission scanning electron micrograph (SEM) (Supra 55-VP, Zeiss) of a typical nanoscale DCE is shown in Figure 1 B, and an optical image of a larger DCE is shown in Figure 1 C.

Electrochemical measurements. A three electrode configuration was used, with two working electrodes (the two electrodes of the probe) and a single Ag/AgCl (silver chloride coated silver wire) quasi reference/counter electrode (QRCE) in the bulk of the solution, as illustrated in Figure 1 D. In G/C mode the potential of one electrode was set to 0.5 V with respect to the QRCE for the diffusion-limited one-electron oxidation of FcTMA^+ to FcTMA^{2+} , and the other electrode was at 0 V with respect to the QRCE for the diffusion-limited one-electron reduction of FcTMA^{2+} . This was achieved in our electrochemical configuration by setting $V_1 = 0.5$ V and $V_2 = -0.5$ V (Figure 1 D). The current at each working electrode was measured using a custom-built high sensitivity bipotentiostat: see Supporting Information, section S5, for a description of the SECM instrument.

Simulations and Theory. Electrochemical measurements provide a quick estimation of the apparent size of an electrode.²⁹ We developed a steady-state three-dimensional FEM simulation of nanoscale (100 nm – 1000 nm) DCEs, based on the probe geometry observed in SEM images of typical nanoscale DCEs (e.g. Figure 1B), to estimate the probe geometry from steady-state diffusion-limited currents. A full description of the FEM simulation, including Figure S1 showing the probe geometry and example diffusion profiles, is given in the Supporting Information, section S6.

The electrodes in the probe are semi-elliptical in shape, and the model is configured so that there are only two independent variables, the major axis size for each of the electrodes.

Thus, in principle, only two current measurements are needed to determine the geometry of the probe.

Platinization of carbon nanoelectrodes. Carbon nanoelectrodes were platinized in a solution of chloroplatinic acid H_2PtCl_6 (2 mM) in 0.1 M sulfuric acid. The reduction of Pt at the carbon nanoelectrode was induced by cycling the potential twice from -1 V to + 0.5 V at a scan rate of 750 mV s^{-1} .

Results and Discussion

DCEs were fabricated with a high success rate (ca. 85 %, based on more than 100 made) on the day of use, with approximately 3 minutes required per tip. A typical DCE (see Figure 1 B and C) consists of two planar semi-elliptical electrodes, separated by a septum and surrounded by glass. The septum size and small surround of glass are typical for probes constructed from theta nanopipets, by the laser pulling technique.^{24,25,38}

Each electrode of a DCE was individually characterized using the steady-state currents for the one-electron oxidation of FcTMA^+ obtained from linear sweep voltammograms. Typical examples for each of the two electrodes of a single probe are shown in Figure 2 A. As expected, the LSVs show a sigmoidal response. Assuming coplanar electrodes, the different magnitude of the limiting currents for each electrode, within an individual probe, indicates that the electrodes are not the same size. Generally, the individual electrodes in a single probe may have slightly different sizes due to asymmetry in the individual barrel sizes in the pulled theta pipet.

This DCE was then used in G/C mode, with the $\text{FcTMA}^{+/2+}$ redox couple. The potential of the generation electrode was swept for the oxidation of FcTMA^+ to FcTMA^{2+} while the potential of the collection electrode was held constant at 0 V for the reduction of any

FcTMA²⁺ back to FcTMA⁺. The resulting generation and collection currents are shown in Figure 2 B. The generation current shows the typical sigmoidal shape, however the magnitude of the limiting current is slightly larger than observed for the single electrode response above, as the second electrode regenerates FcTMA⁺, so providing positive redox feedback to the generator electrode. The collection current shows a similar sigmoidal shape, resulting from the change in local FcTMA²⁺ concentration induced by the generator electrode. The ratio of collection current to generation current defines the collection efficiency, and this probe had a diffusion-limited collection efficiency of ca. 30 %. This reasonable collection efficiency is achieved because the small distance between the two electrodes minimizes diffusional losses.

Nanoscale DCE Characterization. While nanoscale electrodes can be routinely fabricated,^{39,40} the resulting probe geometry is often difficult to determine precisely.²⁹ In principle, it is possible to determine the individual probe geometry for a DCE by SEM after experiments; however, this was found to be problematic due to crystallization of the redox species and supporting electrolyte on the probe. Practically, the estimation of probe geometry is usually achieved by using analytical expressions, or simulations, to relate the experimental current responses to electrode dimension, taking care to avoid pit falls due to non-planar geometrical affects (especially recessed electrodes).^{41–43} More complex geometries, such as the probes used herein, need custom FEM simulations to determine probe geometries from current measurements. A FEM model of the DCE was formulated so that the geometry only depended on the size of the electrode major axes and this allowed the geometry to be determined from only two current measurements.

We calculated the sizes of the nanoscale electrodes in the DCE used to record the data in Figure 2 A and B using the FEM model. First, the geometry was calculated from the diffusion-limited currents at the individual electrodes (Figure 2 A). The probe size (defined

by the size of the major axes) consistent with the diffusion-limited current measured at electrode 1 is shown in blue in Figure 2 C, while the probe size consistent with the measured limiting current for electrode 2 is shown in red. Note that for this model the size of a particular electrode, as determined from its current, shows a weak dependence on the size of the other (unconnected) electrode because changing the size of the latter electrode changes the minor axis size (and also the septum and glass surround width). For example, a smaller unconnected electrode promotes more back diffusion and a slightly higher current at the active electrode. The point at which the two curves in Figure 2 C intersect, 500 ± 50 nm for electrode 1 and 400 ± 25 nm for electrode 2, is the only possible probe geometry, constrained by the model assumptions, which could produce the two individual electrode currents.

The geometry of the probe can also be calculated from the diffusion-limited generation/collection currents, shown in Figure 2 B. With electrode 1 generating FcTMA^{2+} and electrode 2 collecting FcTMA^{2+} (i.e. both electrodes active), the calculated probe size consistent with the measured generation current is shown in blue in Figure 2 D, while the probe size consistent with the measured collection current is shown in red. Again, the point at which these two sets of electrode sizes intersect, electrode 1 major axis of 450 ± 50 nm and electrode 2 major axis of 400 ± 50 nm, was the geometry of the probe, constrained by the model assumptions, calculated from the generation/collection currents. It is evident that the size of electrode 1, from the two geometry calculations 500 ± 50 nm versus 450 ± 50 nm, is reasonably consistent, as is the size of electrode 2, 400 ± 25 nm versus 400 ± 50 nm.

Working surfaces, from which electrode sizes for different currents can be determined, were constructed from the FEM model, and these are shown in the Supporting Information, section S7 (Figure S2). This highlights that the G/C experiments are particularly sensitive to the probe size. In addition, the calculated collection efficiency is shown in Figure 2 E. This shows that probes with similar sized electrodes have collection efficiencies of ca. 30%. A

relative increase in generation electrode size compared to the collection electrode results in a decrease in collection efficiency, while decreasing the generator electrode size increases the collection efficiency.

SECM measurements. DCEs were deployed in SECM to investigate their behavior, in G/C mode, close to surfaces. With FcTMA^+ oxidation at one (generator) electrode and FcTMA^{2+} reduction at the second (collector) electrode, DCEs were translated towards insulating (glass) and conductive (gold) surfaces using IC-SECM mode.³² With IC-SECM the probe is oscillated normal to the surface (in this case with an amplitude of 32 nm at 70 Hz frequency), and damping of the oscillation amplitude is detected when the tip comes into physical intermittent contact with the surface. This mode provides a current-independent means of detecting when the tip and the substrate surface make contact, which is valuable for estimating the distance between the probe tip and the surface during the approach curve measurements.

The DCE generation and collection currents for approaches to glass and gold surfaces are shown in Figure 3 A and B, respectively. The position at which the tip comes into contact with the surface is seen as a sharp drop in the tip position oscillation amplitude, Figure 3 C and D. For convenience, this point is assigned as a distance of 0 μm between the probe electrode and the surface, although in reality, imperfection in the probe alignment and geometry lead to non-zero distances between the active electrodes and the surface.⁴⁴

When approaching to the inert substrate, the generation current decreases, but interestingly the collection current increases, before dropping off when the tip is very close to the substrate. The transient increase in the collection current is because the substrate confines the generated species, FcTMA^{2+} , close to the electrodes, limiting diffusional losses, so leading to enhanced diffusional coupling between the two electrodes. However, once the tip

gets much closer to the inert surface the significant decrease in the generation current, due to the blocking effect of the substrate on the diffusion of FcTMA^+ to the generator, causes the collection current to decrease. On the other hand, Figure 3 E shows clearly that the absolute collection efficiency increases as the distance from the substrate surface decreases. In this plot, the collection efficiency at a particular distance is normalized with respect to that measured in bulk solution.

The approach to a conducting substrate shows that the generation current increases with a decrease of the distance to the substrate (positive feedback),⁴⁵ while the collection electrode is in competition with the substrate and thus as the tip gets closer to the substrate the current at this electrode drops. This competition increases with closer tip/substrate separation and so the collection efficiency decreases monotonically throughout an approach (Figure 3 E). The data in Figure 3 E highlights that the morphology of an SECM collection efficiency approach curve is hugely sensitive to the nature of the substrate, and this provides a route to functional imaging of surface processes, as we demonstrate below.

We now use the FEM model to assess the approach curves. The sizes of the individual electrodes in the probes used for the approach curve experiments was calculated from the steady-state (bulk) generation and collection currents, as described above. For the approach to the insulating surface, the apparent probe dimensions were defined by 120 nm for the generator electrode major axis and 95 nm for the collector electrode major axis, while for the approach to the conducting surface the generator electrode major axis was 160 nm and the collector electrode major axis was 440 nm. Simulation results for approach curves, with the probe perfectly aligned to the surface (which is an approximation as already discussed), to both insulating and conducting substrates were calculated and are shown, in black, in Figure 3 A and B. These show the same topological features as observed in the experimental results, most obviously the increase in collection current when approaching an insulating substrate.

However, quantitative differences are evident between the experimental and simulation results, particularly during the approach to the insulating substrate (Figure 3 A). In this case, the decrease in experimental generator current is apparent at a distance which we would not expect based on the simulation. This suggests that the true probe geometry is larger than determined from the model, and that, in turn, the electrode is recessed. Such recessions are not uncommon in nanoscale electrodes,^{29,46} and quantitative analysis of approach curves is a powerful way of highlighting non-idealized electrode geometries.⁴¹ While we could develop our model to account for misalignment of the probe with respect to the surface and non-ideal geometry this would introduce a number of extra independent parameters, which are not needed for the initial applications herein, in which we seek to demonstrate attributes of DCE generation-collection measurements in a semi-quantitative fashion.

Probing redox reactions at thylakoid membranes. We demonstrate the use of generation-collection measurements to monitor the reactions of an artificial electron acceptor at thylakoid membranes during photosynthesis. The SECM configuration allowed the DCE to be placed close to, but not touching, a monolayer of thylakoid membranes. The DCE, operated in G/C mode, also allowed a flux of the artificial electron acceptor (FcTMA^{2+}) to be generated locally in a controllable manner, and permitted the local flux of both FcTMA^{2+} and FcTMA^+ to be measured concurrently, with good time resolution.

The interaction of electrogenerated FcTMA^{2+} with thylakoid membranes was investigated using the DCE shown in Figure 1 C in G/C mode, as illustrated in Figure 4 A. The probe was placed over a sparse monolayer of thylakoid membranes (a typical surface coverage is indicated in the fluorescence image Figure 4 B) and approached in the dark to the point of maximum collection current, as shown in the approach curve in Figure 4 C. Note that the morphologies of the generator and collector current approach curves are consistent with the thylakoid membrane presenting an inert surface, as discussed above. The probe was then held

stationary while the sample was illuminated using the fluorescence microscope (at a wavelength of 470 nm with an intensity of 3.5×10^{16} photons $\text{s}^{-1} \text{cm}^{-2}$) for a period of 30 seconds and the generation and collection currents during this time were measured. Figure 4 D and E shows, respectively, the relative change in the generation current and collection current during this period. Upon illumination it is apparent that FcTMA^{2+} is reduced to FcTMA^+ at the thylakoid membranes as there is an increase in the magnitude of the generation current and a decrease in the magnitude of the collection current. Interestingly, a steady-state response is quickly reached, with a ca. 30 pA increase in the generation current and a corresponding ca. 30 pA decrease in the collection current. FcTMA^{2+} reduction at the thylakoid membranes ceases immediately when the light is turned off as evidenced by the return to the generation and collection currents to original values. This corresponds to a turnover rate of FcTMA^{2+} to FcTMA^+ of ca. $2 \times 10^8 \text{ s}^{-1}$. An advantage of the DCE probe is that the electron acceptor is generated locally and the spatial resolution is correspondingly high, approximating to the tip size.

To confirm the FcTMA^{2+} reaction with illuminated thylakoid membranes, the herbicide, 3-(3,4-dichlorophenyl)-1,1-dimethylurea (DCMU), which blocks the linear electron transport pathway³⁶ was added. As observed in Figure 4 D and E, the addition of 10 μM DCMU essentially entirely eliminated the light mediated response. This confirms that FcTMA^{2+} is reduced by a component of the photosynthetic electron transport pathway. Interestingly, we can exclude the possibility that FcTMA^{2+} accepts electrons directly from PSII, as is the case, for example, with silicomolybdate, because DCMU inhibits the electron transport pathway after this point.³⁶

Thylakoid membrane imaging. A DCE in G/C mode was used to image a single thylakoid membrane. The probe (generator electrode major axis ca. 1700 nm and collector major axis ca. 700 nm) was placed directly above a single thylakoid membrane at a distance

where the maximum collection current was detected (as above) and then scanned laterally across the sample at a constant height in G/C mode. The sample was illuminated (470 nm, at 3.5×10^{16} photons $\text{s}^{-1} \text{cm}^{-2}$) during the scan to activate the photosynthetic response at the membrane.

A fluorescence image of the thylakoid membrane, due to the auto-fluorescence of chlorophyll, is shown in Figure 5 A. This matches well to the electrochemical images of the thylakoid membrane, one from the generation current (Figure 5 B) and one from the collection current (Figure 5 C), obtained in a single image scan with a DCE. The decrease in generation current over the thylakoid membrane is predominantly the result of local topography features, which is expected as thylakoid membranes are typically 2-4 μm in height. The collection current also decreases over the thylakoid membrane. However, the collection efficiency (Figure 5 D) *decreases* over the thylakoid membrane. This is only possible over an active surface, as shown in the approach curves in Figure 3, and indicates that the thylakoid membranes are actively consuming the electrogenerated FcTMA^{2+} . The effect is very subtle and would be difficult to detect from a single probe SECM feedback measurement, not least because of the convolution of activity and topography in such measurements and the fact that the activity of a single thylakoid membrane is low. Although the substrate generation/tip collection mode might allow the processes to be probed, this would require FcTMA^{2+} in bulk solution and this mode is characterized generally by a significant loss of spatial resolution.^{40,44} In contrast, we see the degree of activity very readily in the collection efficiency image. Although a simple constant height SECM imaging technique was presented here a further important aspect of these probes is that one could use the response of one electrode to sense topography and the other to sense substrate activity.²²

Platinization of carbon nanoelectrodes. Finally, we consider preliminary experiments that show DCEs can be easily and selectively modified, though the selective deposition of Pt

on one electrode while leaving the other one unmodified. Figure S3 in the Supporting Information shows CVs of 1 mM ferrocenemethanol oxidation in aerated solution, for the individual electrodes of a probe, before and after the selective deposition of Pt on one of the electrodes. The deposition of Pt dramatically changes the catalytic properties of the electrode toward oxygen reduction, as can be seen though by the additional oxygen reduction current observed in the negative potential region of Figure S3 B. However, the deposition of Pt does not appreciably change the size of the electrode, as the ferrocenemethanol oxidation limiting current does not change noticeably with the Pt deposition. This highlights the possibility of using DCEs for electrochemical sensing which, with further developments, may allow multicomponent chemical analysis at the nanoscale.

Conclusions

DCEs are simple and quick to fabricate with a wide range of tunable electrode sizes. The probes are well suited to SECM experiments because of the relatively small total size of the end of the probe enabling close positioning to an interface, while the small inter-electrode distance leads to high sensitivity.

For nanoscale DCEs, a FEM model was developed to assist in characterizing the probe size based on simple steady-state limiting current measurements. The electrode sizes were calculated from either single barrel FcTMA⁺ oxidation currents or the G/C currents. This allowed us to estimate the apparent probe geometry from two different measurements and compare them. However, as highlighted in the approach curve measurements, the FEM model does not capture subtle geometric imperfections such as protruding or recessed electrodes, or slight misalignment of the probe. Nonetheless, these initial studies highlight that the probes can be used in a semi-quantitative fashion and, if required, the morphology of

approach curves could be analyzed further to provide additional information on these imperfections.

We have demonstrated that DCEs can be used to interrogate interfaces and surfaces with high sensitivity. DCEs were used to assess local changes in FcTMA^+ and FcTMA^{2+} flux during illumination of thylakoid membranes, and in 2D imaging of a single thylakoid membrane. In both cases, subtle interactions of electrogenerated electron acceptors with the active surface were determined readily through the G/C response.

Further work to extract the geometry from current-based measurements could expand the quantitative capabilities of these probes. In addition, we have shown that individual probes within the DCE can be functionalized, as exemplified by selective deposition of Pt on one electrode while leaving the other one unmodified. Platinized nanoelectrodes have been shown to be promising probes for intra-cellular measurements.⁴⁷ DCEs may thus find applications as single-cell chemical sensors and other modifications are evidently realizable.

Acknowledgement

The authors thank Marc Baghdadi, Neil Ebejer and Robert A. Lazenby for probe fabrication advice, and Alexander Colburn for customized electronics. We thank the ERC (ERC-2009-AdG247143-QUANTIF) for funding for P.R.U, B.P.N. and K.M., and the EPSRC for a MOAC/DTC studentship for K.M. and funding for Y.E.K. and P.A. The University of Warwick is gratefully acknowledged for a Chancellor's International Scholarship for B.P.N. Some equipment used in this research was obtained through Advantage West Midlands (AWM).

Supporting Information

Additional information, as noted in text, on thylakoid membrane sample preparation, probe laser pulling parameters and SECM instruments is available. This material is available free of charge via the Internet at <http://pubs.acs.org>.

References

- (1) Mirkin, V.; Fan, F.; Bard, A. J. *J. Electroanal. Chem.* **1992**, 328, 47–62.
- (2) Mirkin, M. V.; Bard, A. J. *Anal. Chem.* **1992**, 64, 2293–2302.
- (3) Bard, A. J.; Mirkin, M. V.; Unwin, P. R.; Wipf, D. O. *J. Phys. Chem.* **1992**, 96, 1861–1868.
- (4) Zhou, J.; Zu, Y.; Bard, A. J. *J. Electroanal. Chem.* **2000**, 491, 22–29.
- (5) Rodríguez-López, J.; Alpuche-Avilés, M. A.; Bard, A. J. *J. Am. Chem. Soc.* **2008**, 130, 16985–16995.
- (6) Ahmed, S.; Shan, J.; Petrik, L.; Linkov, V. A. *Anal. Sci.* **2004**, 20, 1283–1287.
- (7) Takahashi, Y.; Shevchuk, A. I.; Novak, P.; Murakami, Y.; Shiku, H.; Korchev, Y. E.; Matsue, T. *J. Am. Chem. Soc.* **2010**, 132, 10118–10126.
- (8) Takahashi, Y.; Shevchuk, A. I.; Novak, P.; Babakinejad, B.; Macpherson, J. V.; Unwin, P. R.; Shiku, H.; Gorelik, J.; Klenerman, D.; Korchev, Y. E.; Matsue, T. *Proc. Natl. Acad. Sci. USA* **2012**, 109, 11540–11545.
- (9) Holt, K. B.; Bard, A. J. *Biochemistry-US* **2005**, 44, 13214 – 13223.
- (10) Pierce, D. T.; Unwin, P. R.; Bard, A. J. *Anal. Chem.* **1992**, 64, 1795–1804.
- (11) Tsionsky, M.; Zhou, J.; Amemiya, S.; Fan, F.-R. F.; Bard, A. J.; Dryfe, R. A. W. *Anal. Chem.* **1999**, 71, 4300–4305.
- (12) Amemiya, S.; Bard, A. J. *Anal. Chem.* **2000**, 72, 4940–4948.
- (13) Kueng, A.; Kranz, C.; Mizaikoff, B. *Biosens. Bioelectron.* **2005**, 21, 346–353.
- (14) Matysik, F.-M. *Electrochim. Acta* **1997**, 42, 3113–3116.
- (15) Barnes, E. O.; Lewis, G. E. M.; Dale, S. E. C.; Marken, F.; Compton, R. G. *Analyst* **2012**, 137, 1068–1081.
- (16) Albery, W. J.; Hitchman, M. L. *Ring-Disc Electrodes*; Clarendon Press: Oxford, 1971.
- (17) Slowinska, K.; Feldberg, S. W.; Majda, M. *J. Electroanal. Chem.* **2003**, 554–555, 61–69.
- (18) Zhong, M.; Zhou, J.; Lunte, S. M.; Zhao, G.; Giolando, D. M.; Kirchhoff, J. R. *Anal. Chem.* **1996**, 68, 203–207.
- (19) Liljeroth, P.; Johans, C.; Slevin, C. J.; Quinn, B. M.; Kontturi, K. *Electrochem. Commun.* **2002**, 4, 67–71.

- (20) Fushimi, K.; Matsushita, K.; Hasegawa, Y. *Electrochim. Acta* **2011**, *56*, 9602–9608.
- (21) Yasukawa, T.; Kaya, T.; Matsue, T. *Anal. Chem.* **1999**, *71*, 4637–4641.
- (22) Isik, S.; Etienne, M.; Oni, J.; Blöchl, A.; Reiter, S.; Schuhmann, W. *Anal. Chem.* **2004**, *76*, 6389–6394.
- (23) Gao, N.; Lin, X.; Jia, W.; Zhang, X.; Jin, W. *Talanta* **2007**, *73*, 589–593.
- (24) Yang, C.; Sun, P. *Anal. Chem.* **2009**, *81*, 7496–7500.
- (25) Takahashi, Y.; Shevchuk, A. I.; Novak, P.; Zhang, Y.; Ebejer, N.; Macpherson, J. V.; Unwin, P. R.; Pollard, A. J.; Roy, D. D.; Clifford, C. A.; Shiku, H.; Matsue, T.; Klenerman, D.; Korchev, Y. E. *Angew. Chem. Int. Edit.* **2011**, *50*, 9638–9642.
- (26) Matsue, T.; Koike, S.; Abe, T.; Itabashi, T.; Uchida, I. *Biochim. Biophys. Acta* **1992**, *1101*, 69–72.
- (27) Wong, D. K. Y.; Xu, L. Y. F. *Anal. Chem.* **1995**, *67*, 4086–4090.
- (28) Morton, K. C.; Morris, C. A.; Derylo, M. A.; Thakar, R.; Baker, L. A. *Anal. Chem.* **2011**, *83*, 5447–5452.
- (29) Nogala, W.; Velmurugan, J.; Mirkin, M. V. *Anal. Chem.* **2012**, *84*, 5192–5197.
- (30) Li, Y.; Bergman, D.; Zhang, B. *Anal. Chem.* **2009**, *81*, 5496–5502.
- (31) Cox, J. T.; Zhang, B. *Ann. Rev. Anal. Chem.* **2012**, *5*, 253–272.
- (32) McKelvey, K.; Edwards, M. A.; Unwin, P. R. *Anal. Chem.* **2010**, *82*, 6334–6337.
- (33) McKelvey, K.; Snowden, M. E.; Peruffo, M.; Unwin, P. R. *Anal. Chem.* **2011**, *83*, 6447–6454.
- (34) McGeouch, C.-A.; Peruffo, M.; Edwards, M. A.; Bindley, L. A.; Lazenby, R. A.; Mbogoro, M. M.; McKelvey, K.; Unwin, P. R. *J. Phys. Chem. C* **2012**, *116*, 14892–14899.
- (35) Patten, H. V.; Meadows, K. E.; Hutton, L. A.; Iacobini, J. G.; Battistel, D.; McKelvey, K.; Colburn, A. W.; Newton, M. E.; Macpherson, J. V.; Unwin, P. R. *Angew. Chem. Int. Edit.* **2012**, *51*, 7002–7006.
- (36) Hall, D. O.; Rao, K. K. *Photosynthesis*; Cambridge University Press, 1999.
- (37) Shevela, D.; Messinger, J. *Biochim. Biophys. Acta* **2012**, *1817*, 1208–12.
- (38) Snowden, M. E.; Güell, A. G.; Lai, S. C. S.; McKelvey, K.; Ebejer, N.; O’Connell, M. A.; Colburn, A. W.; Unwin, P. R. *Anal. Chem.* **2012**, *84*, 2483–2491.

- (39) Mirkin, M. V.; Nogala, W.; Velmurugan, J.; Wang, Y. *Phys. Chem. Chem. Phys.* **2011**, *13*, 21196–21212.
- (40) Sun, P.; Laforge, F. O.; Mirkin, M. V. *Phys. Chem. Chem. Phys.* **2007**, *9*, 802–823.
- (41) Sun, P.; Mirkin, M. V. *Anal. Chem.* **2007**, *79*, 5809–5816.
- (42) Wightman, R. M.; Wipf, D. O. In *Electroanalytical Chemistry Vol. 15*; Bard, A. J., Ed.; Marcel Dekker: New York, 1988; pp. 268 – 353.
- (43) Bruckenstein, S.; Janiszewska, J. *J. Electroanal. Chem.* **2002**, *538-539*, 3–12.
- (44) Lazenby, R. A.; McKelvey, K.; Unwin, P. R. *Anal. Chem.* **2013**, *85*, 2937–2944.
- (45) Kwak, J.; Bard, A. J. *Anal. Chem.* **1989**, *61*, 1221–1227.
- (46) Satpati, A. K.; Bard, A. J. *Anal. Chem.* **2012**, *84*, 9498–504.
- (47) Wang, Y.; Noël, J.-M.; Velmurugan, J.; Nogala, W.; Mirkin, M. V.; Lu, C.; Guille Collignon, M.; Lemaître, F.; Amatore, C. *Proc. Natl. Acad. Sci. USA* **2012**, *109*, 11534–11539.

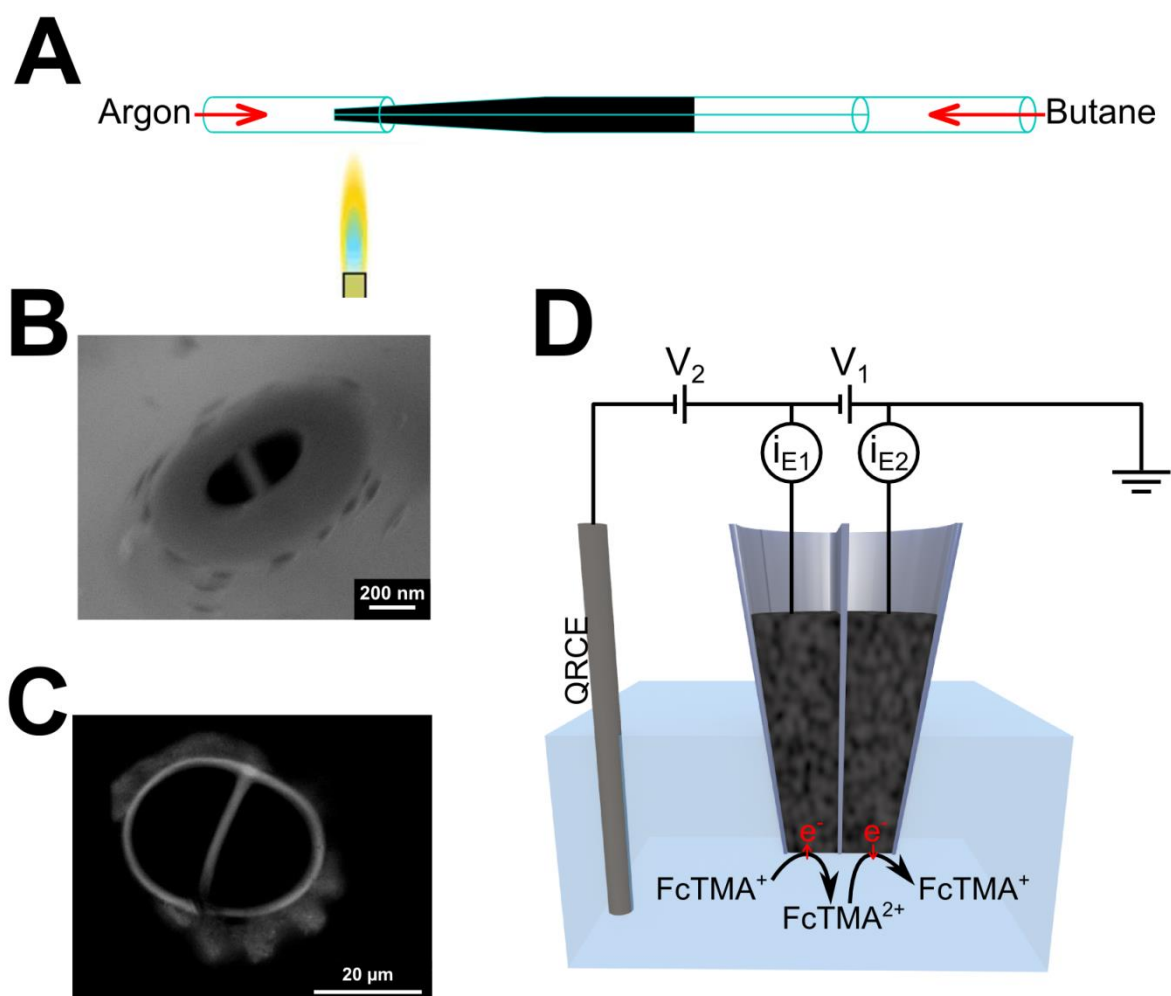


Figure 1

A. Schematic of the carbon deposition step of dual electrode fabrication, in which butane is passed through the pulled quartz theta pipet and pyrolyzed using a hand held butane torch under an argon atmosphere. **B.** SEM of a typical nanoscale DCE. **C.** Optical image of a micron scale DCE. **D.** Schematic of dual electrode configuration, with two working electrodes in the barrels of the probe, and an Ag/AgCl QRCE in solution. The current is measured at each working electrode (i_{E1} and i_{E2}), while the potential of the working electrodes, with respect to the QRCE, is controlled by V_1 and V_2 . In G/C mode FcTMA^+ is oxidized at one electrode to produce FcTMA^{2+} that is reduced at the other electrode.

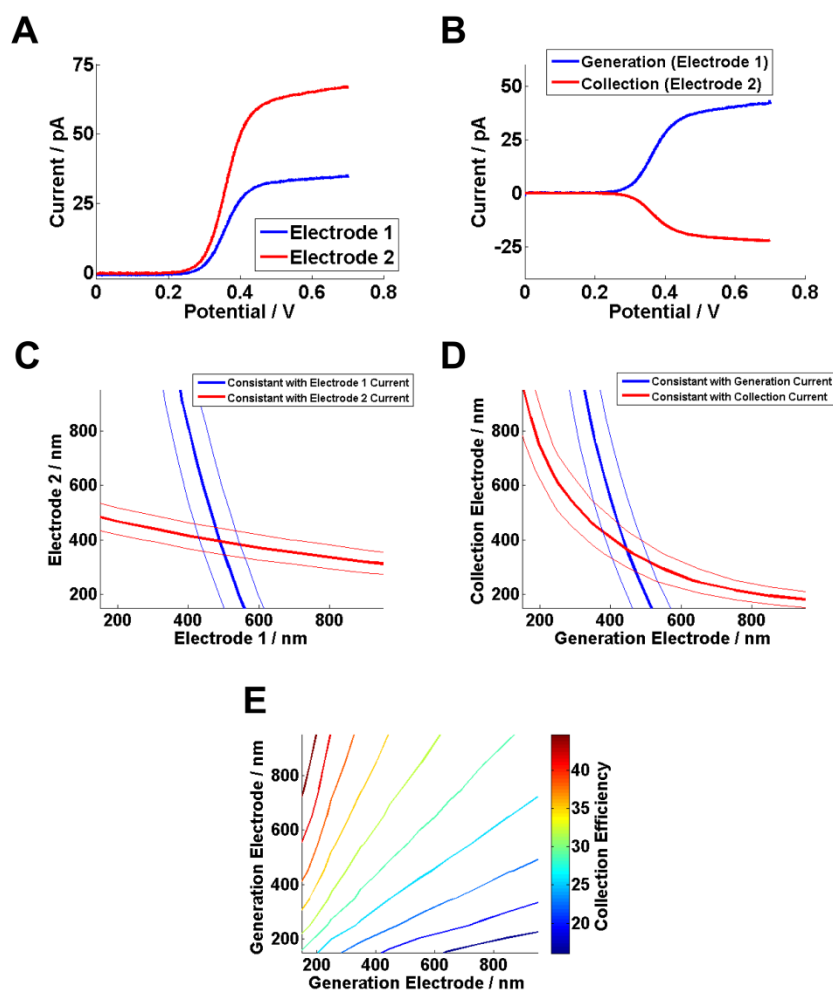


Figure 2

A. LSVs (20 mV s^{-1}) for the oxidation of FcTMA^+ to FcTMA^{2+} at each individual electrode in a nanoscale DCE, while the other electrode was unconnected. **B.** LSVs for the generation and collection currents for $\text{FcTMA}^+/\text{FcTMA}^{2+}$ as the potential of the generator electrode was swept and the collector electrode potential was held at 0 V. **C.** The geometry sets, for electrode 1 in blue and electrode 2 in red, calculated from a FEM model that can generate the single barrel currents. The two geometry sets are consistent with electrode 1 major axis radius $500 \pm 50 \text{ nm}$, and electrode 2 major axis radius $400 \pm 25 \text{ nm}$. **D.** The set of geometries, for electrode 1 in blue and electrode 2 in red, calculated from the FEM model that is consistent with the generation and collection currents. The two are self consistent at electrode 1 major

axis radius 450 ± 50 nm, and electrode 2 major axis radius 400 ± 50 nm. **E.** Collection efficiencies, from simulations, for a range of probe sizes.

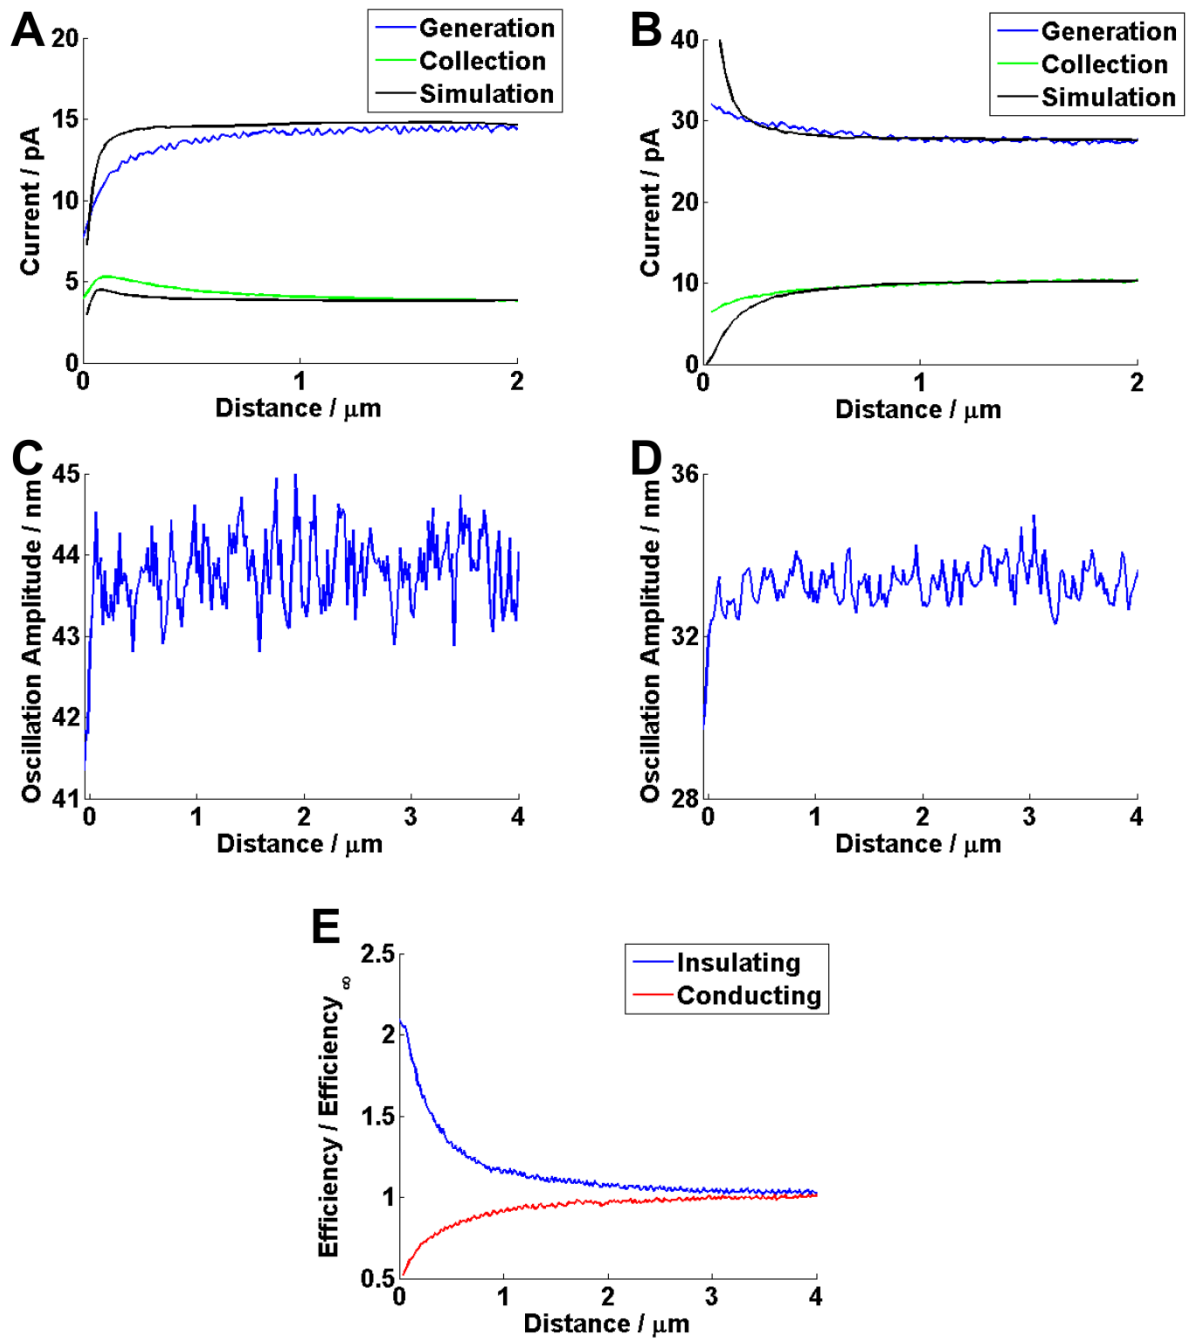


Figure 3

A. Generation and collection currents during the approach of a DCE probe to an insulating (glass) substrate, with the results for a FEM simulation (generation electrode major axis size of 120 nm and collection electrode major axis size of 95 nm) of the same system. **B.**

Generation and collection currents, for an approach to a conducting (gold) substrate, with the results for a FEM simulation (generation electrode major axis size of 160 nm and collection

electrode major axis size of 440 nm). **C** and **D**. Probe oscillation amplitude, showing a sharp decrease that indicates probe contact with the surface, for **A** and **B**, respectively. **E**.

Experimental collection efficiencies for **A** and **B**.

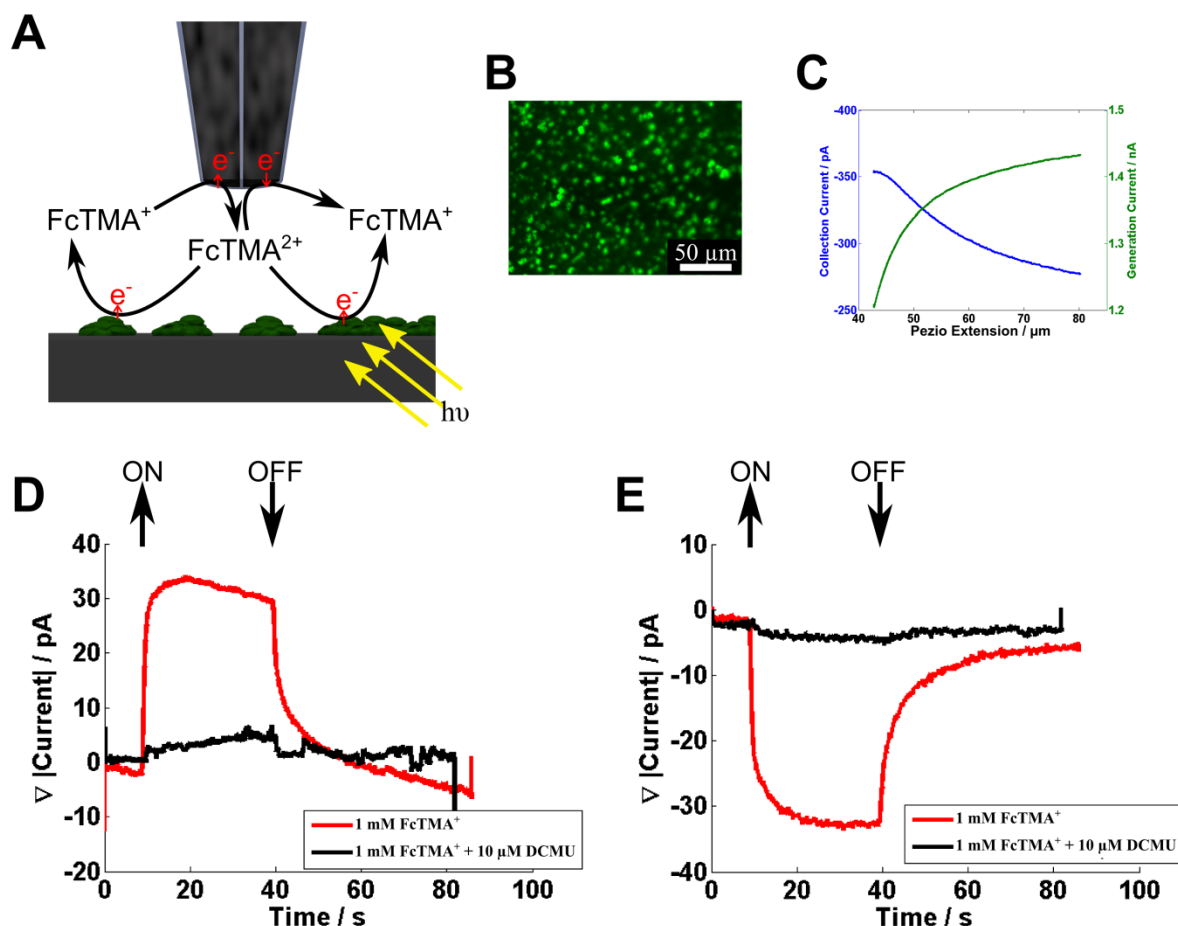


Figure 4

A. Schematic of the DCE in generation/collection mode, with the FcTMA⁺²⁺ couple, above a sparse monolayer of thylakoid membranes. **B.** Fluorescence microscopy image of a sparse monolayer of thylakoid membranes, observed as green spots on the surface. **C.** Approach curves for placing the DCE above the surface containing thylakoid membranes (probe size defined in text). **D.** Generation current response as the monolayer of thylakoid membranes is illuminated with and without DCMU. **E.** Collection current response as the monolayer of thylakoid membranes is illuminated with and without DCMU.

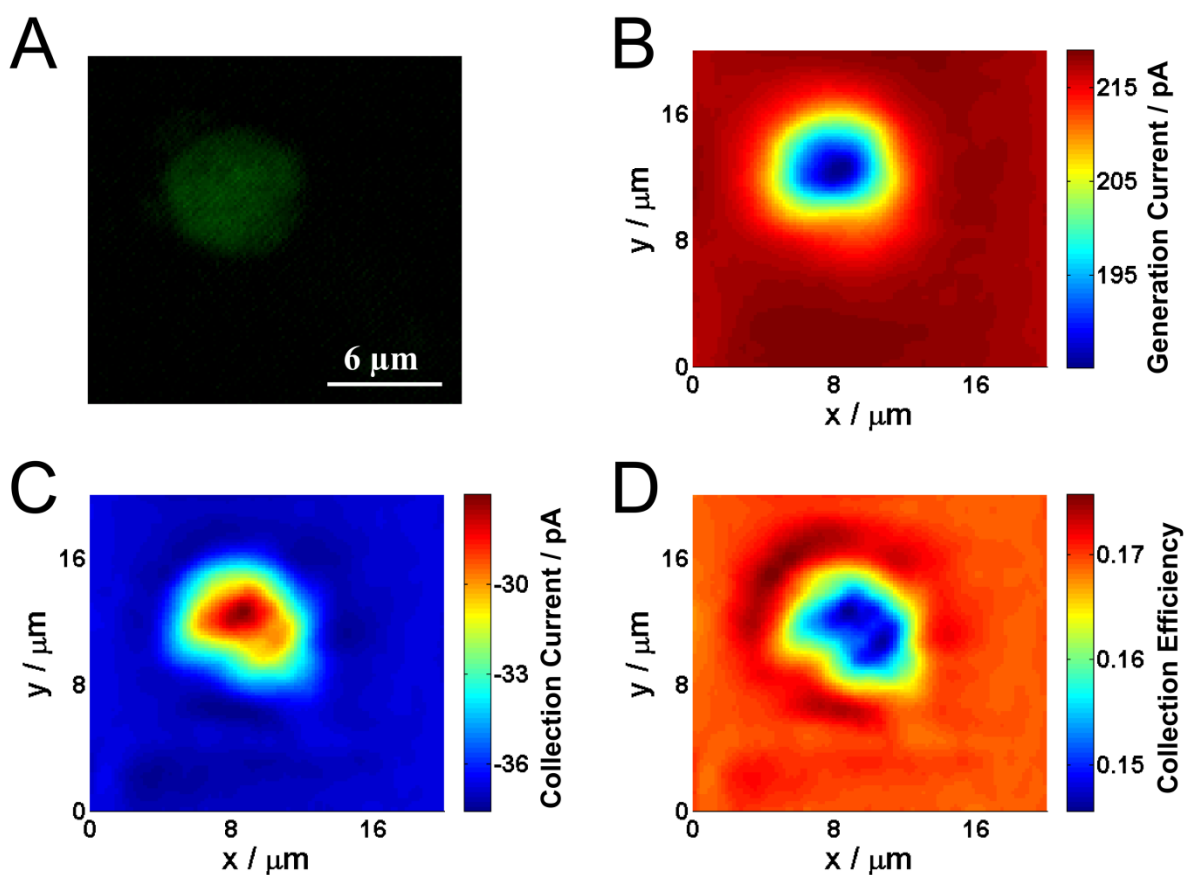


Figure 5

A. Fluorescence image of a single thylakoid membrane. **B.** Generation current (FcTMA^+ oxidation) image of the thylakoid membrane. **C.** Collection current (FcTMA^{2+} reduction) image of the thylakoid membrane. **D.** Collection efficiency image of the thylakoid membrane. The electrochemical images were acquired over a period of 400 seconds.

TOC

